

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307



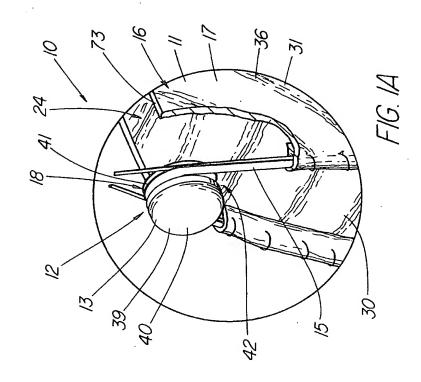

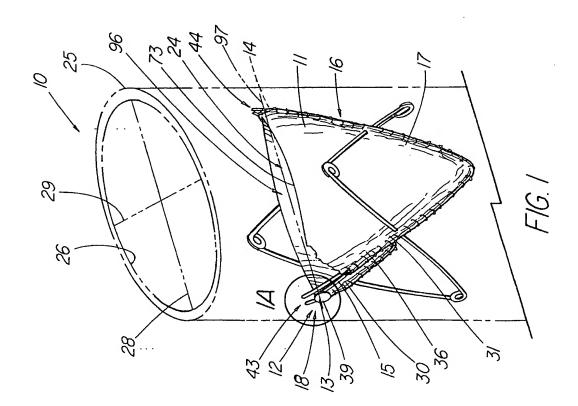

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING

Serial No. 10/787,307




FIG. 2




FIG. 3




FIG. 4






FIG. 5

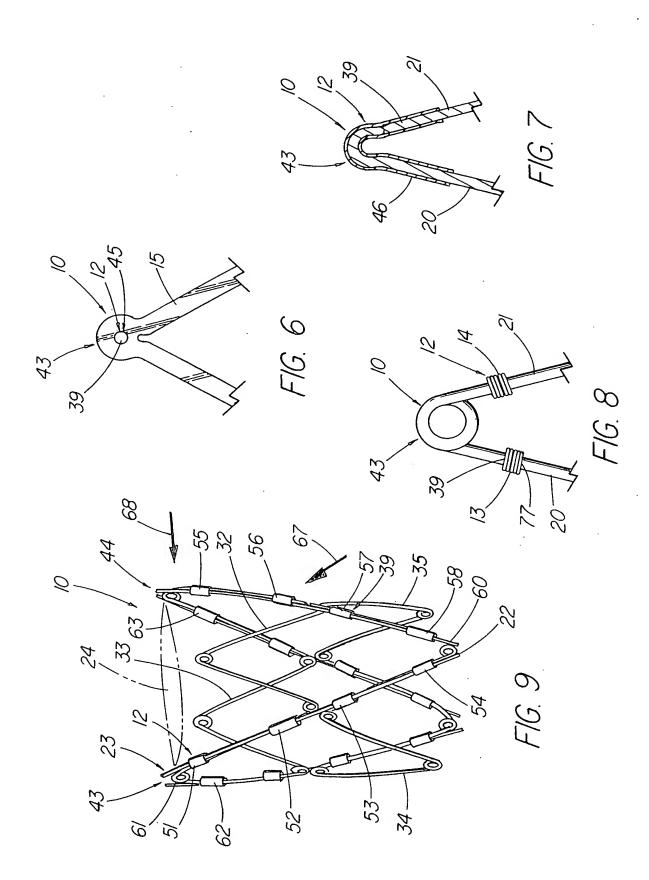


In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER EXTERNAL IMAGING


Serial No. 10/787,307

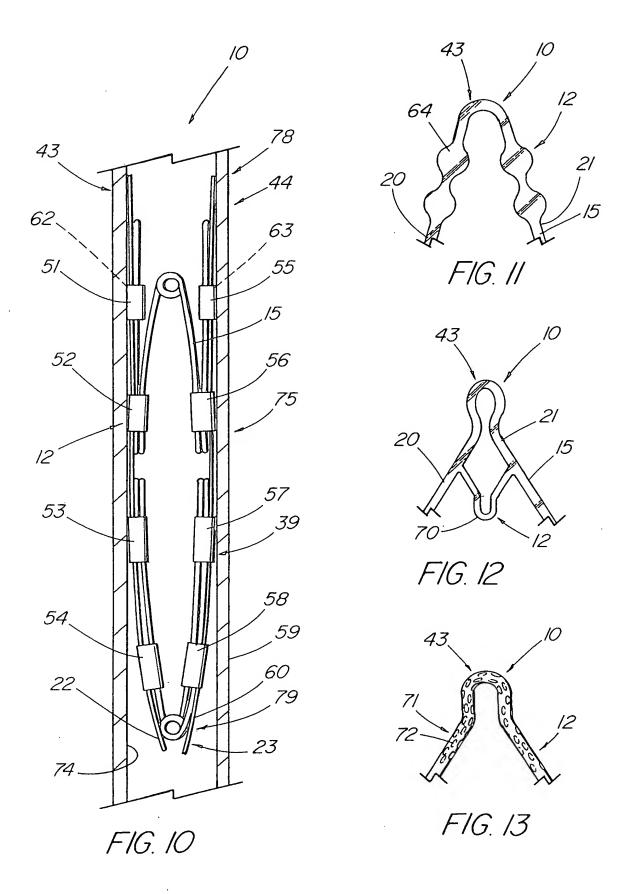




5 of 8 :

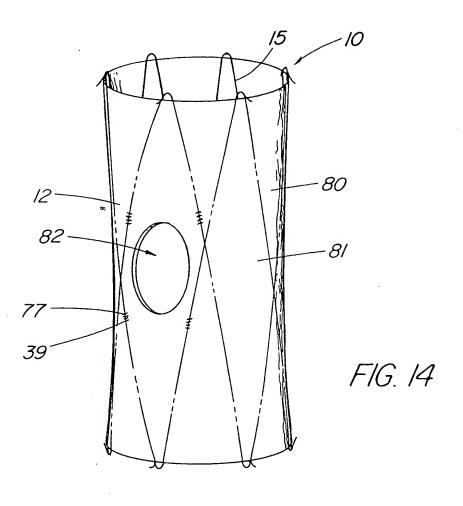

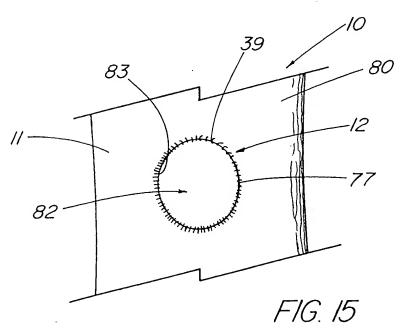


6 of 8


Serial No. 10/787,307

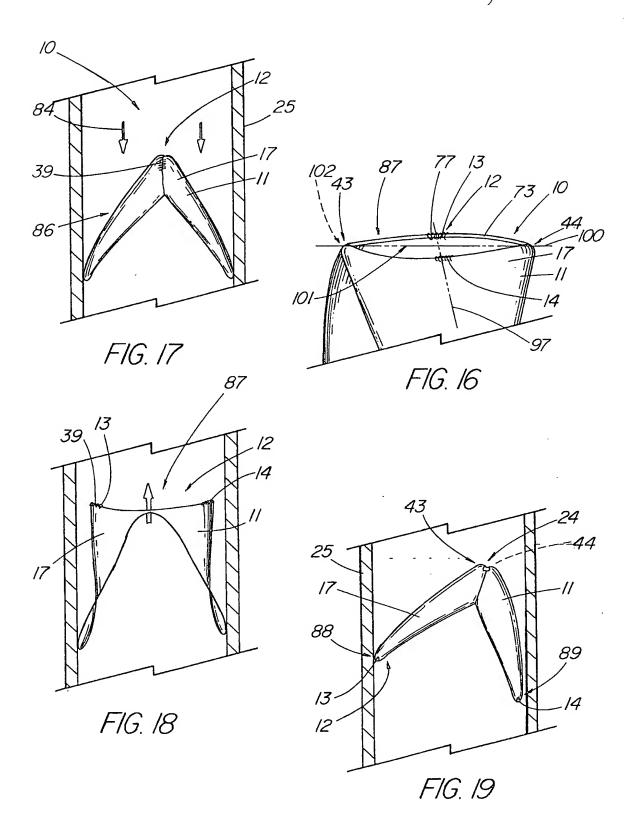

7 of 8

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307

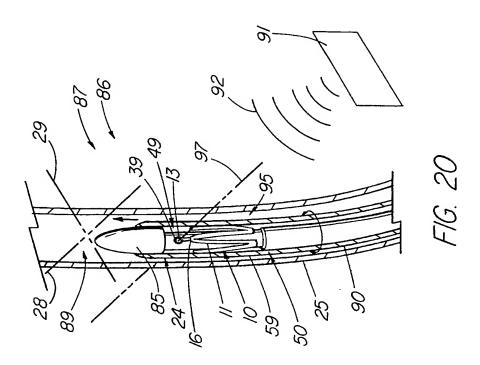

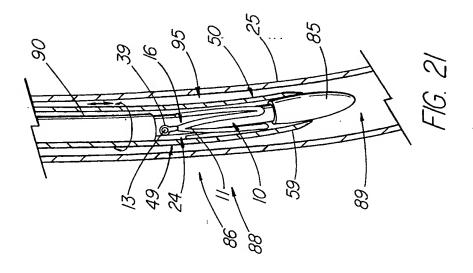



8 of 8

